

PRV

PATENT- OCH REGISTRERINGSVERKET
Patentavdelningen



Intyg Certificate

Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.

This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.

(71) Sökande Siemens-Elema AB, Solna SE
Applicant (s)

(21) Patentansökningsnummer 9904645-0
Patent application number

(86) Ingivningsdatum 1999-12-17
Date of filing

Stockholm, 2000-09-28

För Patent- och registreringsverket
For the Patent- and Registration Office

Åsa Dahlberg

Åsa Dahlberg

Avgift
Fee 170:-

PATENT- OCH
REGISTRERINGSVERKET
SWEDEN

Postadress/Adress
Box 5055
S-102 42 STOCKHOLM

Telefon/Phone
+46 8 782 25 00
Vx 08-782 25 00

Telex
17978
PATOREG S

Telefax
+46 8 666 02 86
08-666 02 86

Description

High Frequency Oscillator Ventilator

The present invention relates to a high frequency oscillator (HFO) ventilator.

- 5 High frequency (HF) ventilators may be classified as belonging to one of two categories, namely the high frequency jet (HFJ) ventilator and the HFO ventilator.

The HFJ ventilator operates to fully ventilate a patient by supplying jet pulses of breathing gas to a patient's airways.
10 These jet pulses are typically supplied through a narrow cannula at a frequency of between 2.5 Hz and 10 Hz, at a pressure of between 0.2 bar and 2.7 bar and with a tidal volume of around 2 to 5 millilitres (ml) per kilogram (kg) body weight of a patient. This high pressure jet pulse causes
15 the lungs to expand during an inspiration phase in which the desired tidal volume is supplied. The expiration phase is essentially passive and results from the natural compliance of the lungs which tends to collapse them and expel the gas. In a modification to this basic HFJ ventilator it is known to
20 provide a Venturi vacuum device in communication with the patient's airways on the expiration side of the ventilator. This device creates a vacuum of typically between 0.002 and 0.025 bar during expiration to promote the natural collapse of the lungs. However expiration is still effectively
25 passive, relying on the compliance of the lungs to push out the supplied gas.

The HFO ventilator operates to fully ventilate a patient by introducing pressure oscillations to a column of gas in communication with a patient's airways. These oscillations
30 cause alternately the supply of breathing gas to and the active extraction of at least the supplied volume of gas from the airways of the patient. It is this active extraction of

the supplied volume that is the primary difference between HFO and HFJ ventilation systems. The peak-to-peak pressure amplitude about a mean airway pressure is typically between 0.05 and 0.2 bar and oscillates at a typical frequency of
5 between 10 Hz and 50 Hz to supply a tidal volume significantly less than required during spontaneous breathing, typically at or around anatomical dead-space volumes, and is usually less than that typically supplied by the jet device during HFJ ventilation.

10 Both types of HF ventilator operate in marked contrast to a known conventional mechanical ventilator. The conventional ventilator operates to fully ventilate a patient by supplying breathing gas to the patient's airways in an amount and at a frequency substantially equal to those of a spontaneously
15 breathing patient. Typically then, for an adult, the conventional mechanical ventilator will provide a tidal volume of around 500 millilitres at a frequency of around 0.2Hz.

The HFO ventilator generally comprises a gas conduit having
20 an opening at one end for connection to the patient's airways and an opposite end provided in gas communication with an oscillator. The oscillator includes a reciprocally moveable element, such as a membrane or a piston, as part of a variable gas holding volume to which the end of the conduit
25 is in gas communication. A drive unit is provided to reciprocate the moveable element at a predetermined high frequency to alternately remove a volume of gas from and return it to the gas conduit. Over- and under- pressure pulses are thereby supplied to gas within the conduit at that
30 frequency. This causes a column of gas, the volume of which is dependent on the volume change of the oscillator, to be moved along the gas conduit into and out of the patient's airway and thereby provide ventilation. A continuous so called 'bias' flow of fresh breathing gas moves along a flow

path between an inlet and an outlet and intersects the path of the moving column within the conduit to flush through the outlet carbon dioxide rich gas that has passed from the patient's lungs. This bias flow also maintains a mean positive airway pressure (or bias) about which pressure the high frequency pressure pulses oscillate. However, a disadvantage with the known HFO ventilator is that a large percentage (typically over 70%) of the volume of gas moved by the variation in oscillator volume never reaches the patient and is lost from the conduit through the outlet. The volume change of the oscillator must therefore be made commensurately larger in order to supply an adequate tidal volume to the patient. As a result it becomes increasingly difficult to maintain the necessary volume changes as the oscillation frequency increases and tidal volumes may then become insufficient. An additional problem is that the gas conduit itself must be made of a relatively stiff material so that the energy of the pressure pulses generated by the oscillator is not reduced through work done in expanding and contracting the conduit. Such a length of stiff conduit makes the HFO ventilator cumbersome to deploy.

According to the present invention there is provided an HFO ventilator described in and characterised by the present claim 1. In generating oscillations by alternately introducing and withdrawing a volume of additional gas sufficient to provide a desired tidal volume to the patient's airways the disadvantage of reciprocating the large moveable element of the known HFO ventilator is removed.

Preferably, the oscillator may be adapted to introduce the additional gas proximal the opening in the first gas conduit which is intended for connection with the patient's airways. This reduces dead-space, allows a more flexible tubing to be used for the remainder of the conduit away from the opening without the risk of energy being lost in expanding and

contracting the tubing and permits smaller volumes of gas to be used in order to generate the desired pressure oscillations.

Conveniently, the additional gas may be introduced by a pulse generator via a second conduit which opens into the first and its removal may be by a separate device via the first, the second or even a third conduit. The increased design flexibility provided by providing separate means for introducing and for removing gas also allows each of the means to be optimised for its intended purpose.

Exemplary embodiments of the present invention will now be described with the aid of and reference to the drawings of the accompanying figures, of which:

Fig. 1 shows a first embodiment of an HFO ventilator according to the present invention.

Fig. 2 shows a second embodiment of an HFO ventilator according to the present invention.

Fig. 3 shows a third embodiment of an HFO ventilator according to the present invention.

Considering now Fig. 1, an HFO ventilator 2 is shown in operative connection to a source of pressurised breathing gas 4. The HFO ventilator 2 is configured to utilise the source of breathing gas 4 both as a bias flow and as a source of an additional gas, as will be described below. The HFO ventilator 2 is provided with a primary conduit 6 that has at one end a patient opening 8 which is intended to be placed in gas communication with a patient's airways, for example by connection to a conventional endotracheal tube (not shown). A vent opening 10 is also provided in the primary conduit 6 through which gas may be vented to atmosphere (as shown) or to a known gas recovery means (not shown). A one-way valve 12

is disposed within the primary conduit 6, proximal the vent opening 10 and is configured to prevent gas entering the conduit 6 through the vent opening 10. A variable aperture throttle valve 14 is also disposed in the primary conduit 6 at a location proximal the one-way valve 12. A bias gas flow inlet 16 is connectable to the source of pressurised breathing gas 4 via a pressure regulator 18 and is connected to the primary conduit 6 at a location proximal the patient opening 8. A secondary conduit 20 terminates with an opening 22 in the primary conduit 6 proximal to and directed towards the patient opening 8. A solenoid valve 24 switchably connects the secondary conduit 20 either to an extraction device 26, such as a rotary or reciprocatory vacuum pump, or to a conditioning device 28. The extraction device 26 is vented to atmosphere (or alternatively to a gas recovery means) and the conditioning device 28 is connected to the source of pressurised breathing gas 4 via a pressure regulator 30. A control signal generator 32 is operably connected to the solenoid valve 24 to provide it with control signal pulses which cause the valve 24 to alternately connect the conditioning device 28 and the extraction device 26 to the secondary conduit 20 at a predetermined and preferably variable frequency which is typically between 10 and 50 Hz. As a safety feature, the solenoid valve 24 may be adapted to remain in a "neutral" state in the absence of a control signal from the signal generator 32 in which state neither of the devices 26,28 are connected to the secondary conduit 20. The supply of an alternating positive and a negative signal from the control signal generator 32, such as a sine or square wave signal, can then cause the solenoid valve 24 to connect respectively the conditioning device 28 or the extraction device 26 to the secondary conduit 20 in an alternating manner dependent on the polarity of the supplied signal.

During the use of the HFO ventilator 2 a continuous bias gas flow is provided by gas from the source 4, through the primary conduit 6 between the inlet 16 and the vent opening 10. This establishes a mean airway pressure within a patient's airways which maintains the patient's lungs in a partially inflated condition throughout ventilation. The mean airway pressure may be regulated by adjusting one or both of the pressure regulator 18 and the aperture 34 of the throttle valve 14. Gas from the source 4 also passes through a different pressure regulator 30 to a conditioning device 28 where moisture may added and/or the moist gas warmed. The solenoid valve 24 is operated in response to electrical pulses from the control signal generator 32 to periodically connect the moist gas from the conditioning device 28 to the secondary conduit 20 in order to generate gas pulses at a predetermined frequency and for a predetermined time. In this manner pulses of additional fresh gas are introduced into the primary conduit through the opening 22 in the secondary conduit 20. Because of relative dispositions of the opening 22, the patient opening 8 and the bias gas inlet 16 then each pulse need only consist of a volume of gas substantially equal to the tidal volume necessary to provide adequate ventilation at the operating frequency of the HFO ventilator. As with the known HFO ventilator this desired tidal volume may be calculated as being between one and four ml per kg body weight of the patient. This additional gas induces a pressure increase in the gas within the primary conduit 6 similar to that associated with the known HFO ventilator. This causes a similar volume of gas to be moved through the patient opening 8 and to the patient's lungs where gas exchange occurs to move oxygen (O_2) into the lungs and carbon dioxide (CO_2) into the gas. After the delivery of each pulse the signal from the signal generator 32 causes the solenoid valve 24 to connect the extraction device 26 to the conduit 20 for a predetermined time so as to withdraw through the

opening 22 at least the same volume of gas which was pushed out of the patient opening 8 by the immediately preceding pulse of additional gas. This induces a pressure decrease in the gas within the primary conduit and causes a similar
5 volume of gas to be moved out of the patients lungs. Gas entering the primary conduit through the patient opening 8 is relatively rich in CO₂ and is flushed from the system through the one-way valve 12 by the bias gas flowing from the inlet 16 to the vent opening 10.

10 Considering now Fig. 2, an HFO ventilator 36 is shown in operative connection to a first source of pressurised breathing gas 38 which in use will act as an additional gas source and to a second source of pressurised breathing gas 40
15 which in use will act as a bias gas supply. The HFO ventilator 36 comprises a primary conduit 42 that has at one end a patient opening 44 which is intended to be placed in gas communication with a patient's airways, for example by connection to a conventional endotracheal tube (not shown). A
20 mushroom valve 46 terminates a vent opening 48 in the primary conduit 42. A bias gas flow inlet 50 is connectable to the bias gas flow supply 40 so that a continuous flow of bias gas may be introduced into the primary conduit 42 proximal the patient opening 44 and which exits via the vent opening 48 when the pressure within the conduit 42 exceeds the closing
25 bias of the mushroom valve 46. This pressure is then the mean airway pressure established by the HFO ventilator 36 in use. A side branch 52 of the primary conduit 42 connects to a gas pulse generator 54 through a one-way valve 56 which is
30 arranged so that gas can only flow from the gas pulse generator 52. The gas pulse generator 54 comprises a first variable gas holding volume 58 having a reciprocally moveable element, here a piston 60, as one wall and an inlet 62 connected to the source of additional gas 38. A first drive unit 64 is included to reciprocate the piston 60 at a
35 predetermined high frequency in dependence of a signal output

from a control signal generator 68. The control signal generator 68 is also arranged to supply a control signal to a second drive unit 70 which is operably connected to a piston 72 of a second variable gas holding volume 74 of an extraction device 76. The second variable gas holding volume 74 is provided with a vent 78 which is here shown to connect to atmosphere via a one-way valve 80. A further side branch 82 connects the second variable volume 74 to the primary conduit 42 via a one-way valve 84. The two one-way valves 80,84 are mutually arranged so that gas can only flow from the side branch 82 and out of the vent 78 as the piston 72 is reciprocated.

The HFO ventilator 36 operates broadly as described in respect of the HFO ventilator 2 of Fig. 1. Thus, in use, a bias flow is provided between the inlet 50 and the vent opening 48 to pressurise gas within the primary conduit 42 and a patient's airways until a mean airway pressure is established which is dependent on the opening pressure of the mushroom valve 46. A pulse of additional gas is supplied to the primary conduit 42 by the gas pulse generator 54 so as to intersect the flow path of the bias gas. The gas pulse is generated as the piston 60 is moved to reduce the volume of the variable gas holding volume 58 and thereby force gas out of the connecting side branch 52. As the piston 60 is moved to increase the volume of the variable gas holding volume 58 fresh gas is supplied to that volume 58 from the gas source 38. Alternately with the supply of the additional gas pulse by the generator 54 gas is withdrawn from the primary conduit 42 by the extraction device 76. The piston 72 is moved to increase the volume of the second variable gas holding volume 74 and thereby suck in gas from the conduit 42. As the piston 72 is moved in the opposite direction gas is forced from the variable volume 74 through the vent 78. As described above in connection with the ventilator 2 of Fig. 1, the alternating supply to and withdrawal from the primary

conduit 42 of a volume of gas causes oscillations in the column of gas within the conduit 42 (and consequently within a patient's lungs) at a frequency dependent on the frequency of reciprocation of the pistons 60,72.

5 The control signal generator 68 may be usefully adapted to provide an independently variable signal to each of the piston drive units 64,70 so that at least the phase difference between each the control signals may be varied. In this way withdrawal of the gas by the extraction device 76
10 may begin slightly before the end of the delivery of the gas pulse by the generator 54 to provide a smooth transition between supply and withdrawal of gas. This also allows delays caused by differences, for example in length, of conduits connecting the gas pulse generator 54 and the extraction
15 device 76 to the primary conduit 42, to be compensated for.

Additionally the stroke lengths of the two pistons 60,72 may different and variable to allow more gas to be withdrawn than was supplied. The bias flow can be adjusted to compensate for this net loss of gas from the primary conduit 42 which
20 promotes the removal of CO₂ from the ventilator 36.

Considering now Fig. 3, an HFO ventilator 86 is shown having a primary gas conduit 88 with a patient opening 90 at one end and with an opening 92 at the opposite end connected to an extraction device 94. The extraction device 94 comprises a
25 variable gas holding volume 96 which has a reciprocally moveable element, again shown as a piston 98, as a defining wall section. The piston 98 connects to a drive unit 100 which reciprocates the piston 98 at an operating frequency of the HFO ventilator 86 in dependence of an oscillating control
30 signal provided by the control signal generator 102. A bias gas flow inlet 104 connects to the inside of the primary conduit 88 at a location proximal the patient opening 90 and a gas outlet 106 connects to the inside of the primary

conduit 88 at a location distal the patient opening 90 and in gas communication with the variable gas holding volume 96. The inlet 104 and outlet 106 are disposed to define a flow path there between for bias gas within the primary conduit 88. A one-way valve 108, for example a mushroom valve, is located at the gas outlet 106 and arranged to allow the only the venting of gas from the primary conduit 88. This valve 108 is adapted to open only when pressure within the primary conduit 88 reaches a predetermined and possibly adjustable level. In this way a desired mean airway pressure may be established by the HFO ventilator 86. A further one-way valve 110 is located within the primary conduit 88 to prevent gas passing from the variable volume 96 and through the patient opening 90 as the piston 98 is moved to reduce the volume of the variable volume 96. A secondary conduit is provided with an opening 114 in the primary conduit 88 through which gas may be directed to intersect the bias flow path and move towards the patient opening 90. A gas pulse generator 116 comprises a controllable on/off valve 118 which is switched under the control of the control signal generator 102 to alternately allow and prevent passage of gas from a pressurised source of an additional gas (not shown) which connects to an inlet 120 of the gas pulse generator 116. Also provided within the gas pulse generator 116, in-line between the inlet 120 and the valve 118, is a humidifier 122 which conditions the additional gas before it is supplied to the primary conduit 88.

In use the control signal generator 102 actuates the on/off valve 118 and the piston 98 in a timed relationship to alternately supply a pulse of gas to and withdraw gas from the primary conduit 88 and thereby oscillate gas therein at the desired operating frequency of the HFO ventilator and thereby effect ventilation of a patient.

It will be appreciated by those skilled in the art that non-inventive modifications may be made to the embodiments of Figs. 1 to 3 or other embodiments devised whilst remaining within the scope of the invention as claimed. Thus, for
5 example, whilst it is preferable to introduce the bias flow into the primary conduit 42 proximal the patient opening 44 this flow may be introduced distal the opening 44 and extracted proximal it. Additionally, the size variable gas
10 holding volumes 58,74,96 may be of a known type other than a piston arrangement and may comprise a mechanically, pneumatically or electro-mechanically driven diaphragm or collapsible wall section.

9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
2187
2188
2189
2190
2191
2192
2193
2194
2195
2196
2197
2198
2199
2200
2201
2202
2203
2204
2205
2206

Claims

1. A high frequency oscillator (HFO) ventilator (2;36;86) comprising a first gas conduit (6;42;88) having an opening (8;44;90) for gas connection with a patient's airways and a bias gas flow inlet (16;50;104) and outlet (10;48;106) disposed to define there between a flow path for a bias gas within the first conduit (6;42;88); and an oscillator operable to induce pressure oscillations in gas within the first conduit (6;42;88) to move gas along a path intersecting the flow path for a bias gas alternately into and out of the opening (8;44;90) at a predetermined high frequency; characterised in that the oscillator comprises means (24,26;54,76;116,94) for alternately introducing a volume of additional gas into and withdrawing at least the volume of gas from the first gas conduit (6;42;88) to induce the pressure oscillations.

2. An HFO ventilator as claimed in claim 1 characterised in that the oscillator is adapted to introduce the volume of additional gas into the first gas conduit (6;42;88) to intersect the bias flow path at a location proximal the opening.

3. An HFO ventilator as claimed in claim 1 or claim 2 characterised in that the means comprises a gas pulse generator (24;54;116) adapted to supply to a second gas conduit (20;52;112) arranged to introduce additional gas into the first gas conduit (6;42;88) in a direction towards the opening (8;44;90) a train of gas pulses wherein each pulse contains the volume of additional gas and is separated from a next pulse in the pulse train by an inter-pulse interval; and an extraction device (24,26;76;94) operable to withdraw gas from the first gas conduit (6;42;88) at least in each inter-pulse interval.

4. An HFO ventilator as claimed in claim 3 characterised in that the extraction device (24,26) is arranged in gas communication with the second gas conduit (20) to withdraw the gas therethrough.

5. An HFO ventilator as claimed in claim 3 characterised in that the extraction device (76) is arranged in gas communication with the first gas conduit (42) via a third gas conduit (82) through which the device (76) withdraws the gas.

10 6. An HFO ventilator as claimed in claim 3 characterised in that the extraction device (94) is arranged in gas communication with an end (92) of the primary gas conduit (88) distal the opening (90).

15 7. An HFO ventilator as claimed in claim 6 characterised in that the extraction device (96) is further co-operatively arranged in gas communication with the bias flow outlet (106) to vent the withdrawn gas therethrough.

20 8. An HFO ventilator as claimed in any of the claims 3 to 7 characterised in that the extraction device (76;94) comprises a size variable gas holding volume (74;96) arranged in gas communication with the first gas conduit (42;88), the gas holding volume (74;96) being defined at least in part by a wall section (72;98) reciprocally moveable
25 in timed relationship with the operation of the gas pulse generator (54;116) to alternately increase the size of the gas holding volume (74;96) to withdraw gas from the first conduit (42;88) at least during an inter-pulse interval and to decrease the size of the gas holding volume (74;96) to
30 vent the withdrawn gas during a next gas pulse of the pulse train.

9. An HFO ventilator as claimed in any preceding claim characterised in that the oscillator is adapted to introduce a volume of gas of between one and four millilitres per kilogram weight of the patient as the volume
5 of additional gas.



Abstract

High Frequency Oscillator Ventilator

A high frequency oscillator (HFO) ventilator (2) comprises a first gas conduit (6) having an opening (8) for gas connection with a patient's airways and a bias gas flow inlet (16) and outlet (10) disposed to define therebetween a flow path for a bias gas within the first conduit (6). An oscillator comprises means (24,26) operable to alternately introduce a volume of additional gas from a source (4) into and withdrawing at least the same volume of gas from the first gas conduit (6) thereby inducing pressure oscillations in gas within the first conduit (6) to move gas along a path intersecting the flow path for a bias gas alternately into and out of the opening (8) at a predetermined high frequency dependent on the output of a control signal generator (32).

Fig. 1

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32

1/3

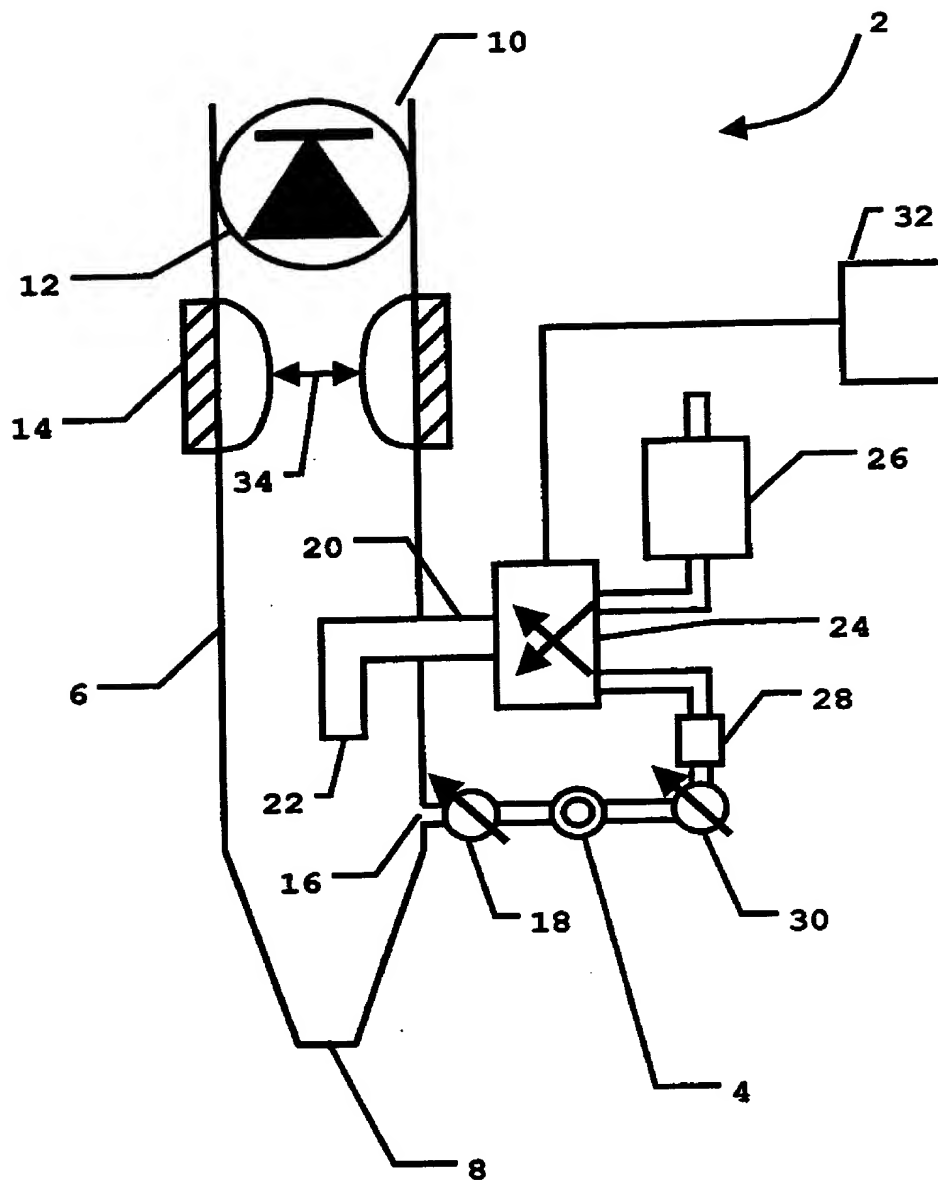


FIG. 1

2/3

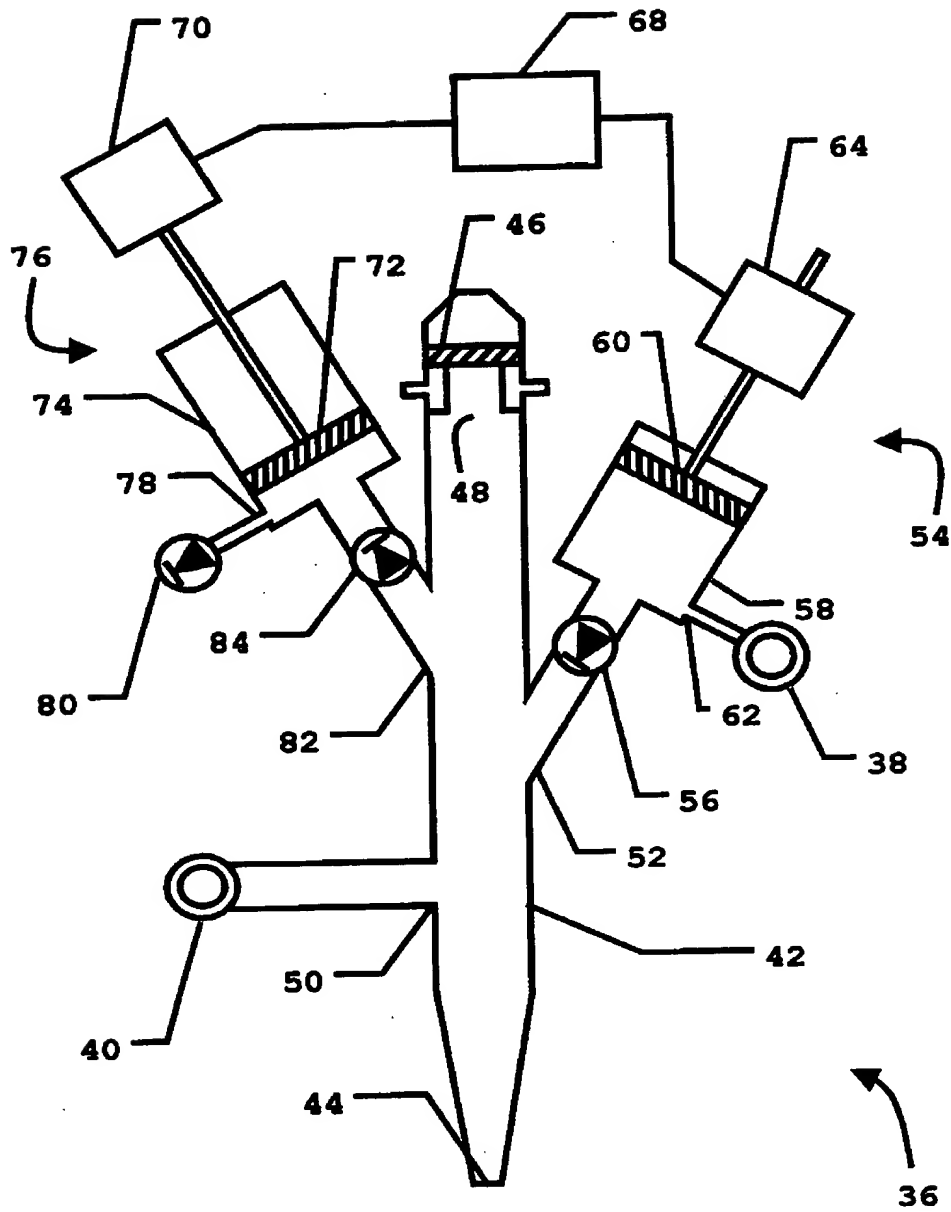


FIG. 2

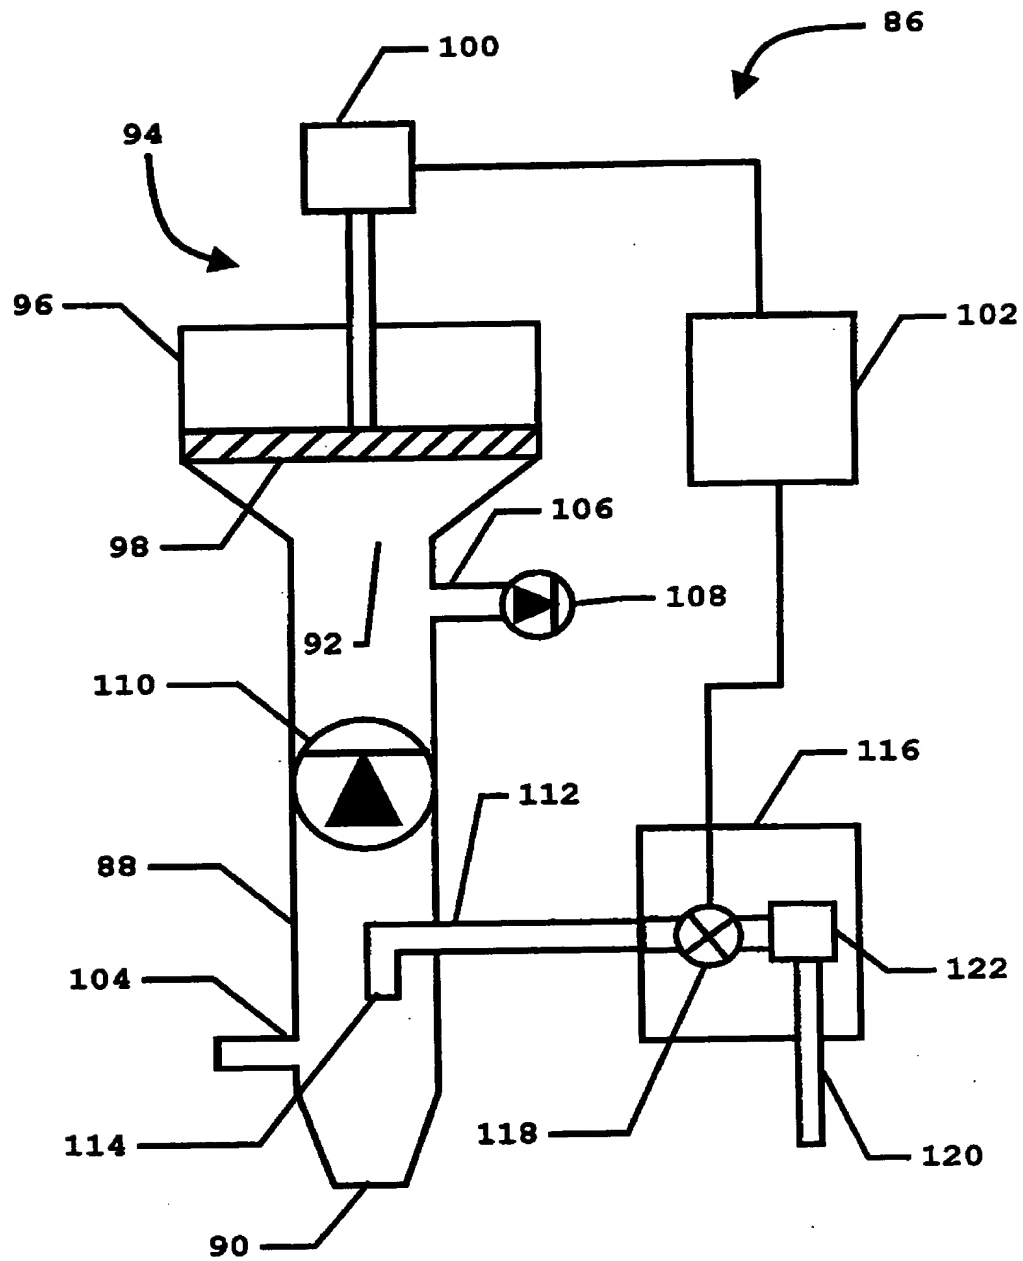


FIG. 3